

Slicer annotations for the Quantitative Imaging Network

Andrey Fedorov

10 Jan 2012

QIN

- 13 centers of imaging excellence:
 - <https://wiki.nci.nih.gov/display/CIP/QIN>
- Goal: to promote research and development of quantitative imaging methods for the measurement of tumor response to therapies in clinical trial settings, with the overall goal of facilitating clinical decision making
- *Support creation of public registries and image database resources to support clinical decision making for therapies by the broader oncology community*

Scope of work

- Supplement to BWH QIN grant
- “implement support of AIM in 3D Slicer, including storage of annotations produced by 3D Slicer in AIM format and importing AIM annotations into 3D Slicer.”

Why DICOM SR/AIM?

- “Structure” of most common radiologic reports: “Finding” and “Impression” sections dictated
- Difficult to use for research, data mining, confusion possible even while exchanging reports among radiologists
- No explicit connection of the report to the image finding
- Need structure, vocabulary, connection to the finding in the image


DICOM SR basics

- Designed to be self-describing information structure
- Support templates and context-dependent terminology
- DICOM Supplement 23
- Supported by vendors
 - Siemens Syngo.via
 - Others?

Tree of content

C.Z.4 SR Content Tree Example (Informative)


Figure C.Z.4-1 depicts the content of an example diagnostic interpretation.

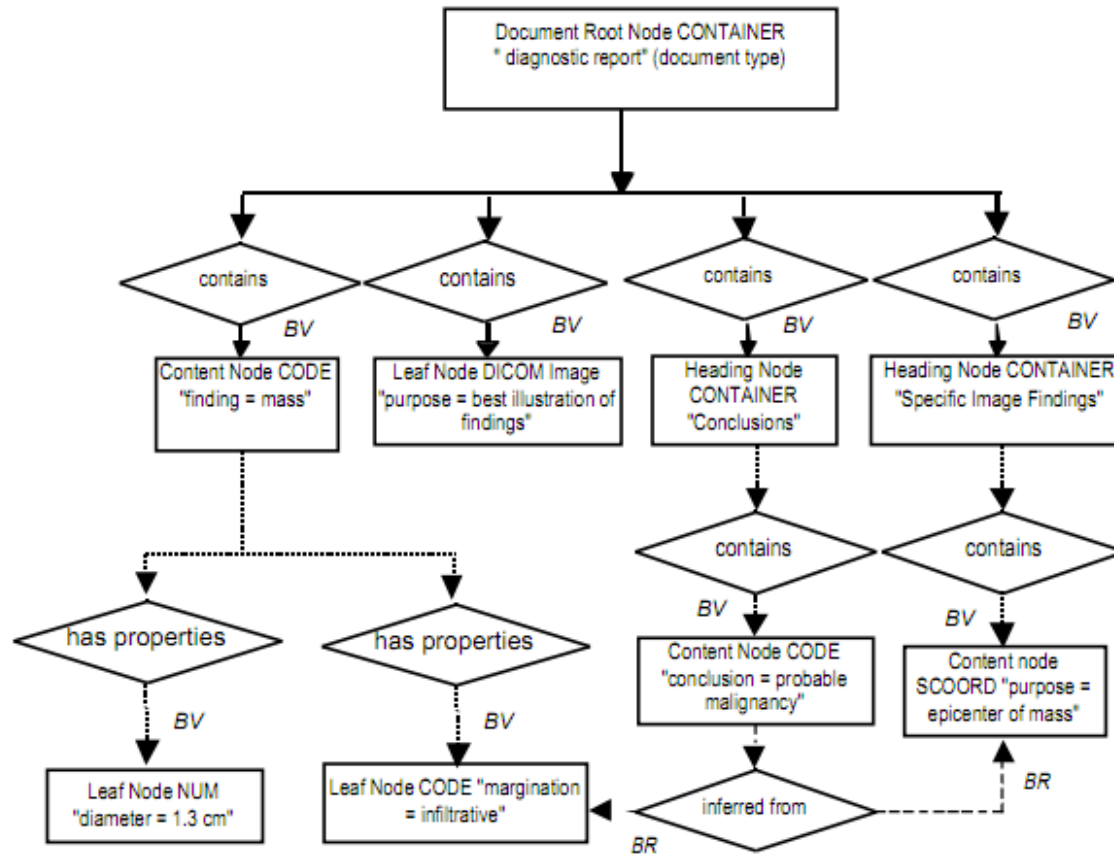

* Relationship Modes
BV = By-value
BR = By-reference

Clinical user view

Chest X-ray Report:
Observer: Clunie^David^A^Dr.
History: malignant melanoma excised 1Y
Findings:
- finding: multiple masses in both lung fields
- best illustration of findings:
Conclusions:
- conclusion: cannon-ball metastases
- conclusion: recurrent malignant melanoma
Diagnosis Codes:
- diagnosis: 172.9/ICD9
- diagnosis: 197.0/ICD9



The image is a black and white chest X-ray showing the lungs, heart, and spine. A black circle is drawn around a mass in the right lung field, and a black arrow points from the text 'best illustration of findings:' to this circle. The X-ray shows multiple masses in both lung fields, consistent with the findings described in the report.

FIGURE 1. Simple example of a DICOM Structured Report

Tree elements

- Value types (CONTAINER, CODE, TEXT, SCOORD)
- Relationships (“contains”, “has properties”, “inferred from”)
- Markup: SCOORD
 - POINT, MULTIPOINT, POLYLINE, CIRCLE, ELLIPSE
 - Pixel coordinates
 - POLYLINE is always closed!

Annotation Image Markup (AIM) basics

- Information model
- Described by XML schema
- Serialized using XML
- Terminology:
 - An image *annotation* is the explanatory or descriptive information about the pixel data of an image that is generated by a human or machine observer.
 - An image *markup* is the graphical symbols placed over the image to depict an annotation.

AIM Markup

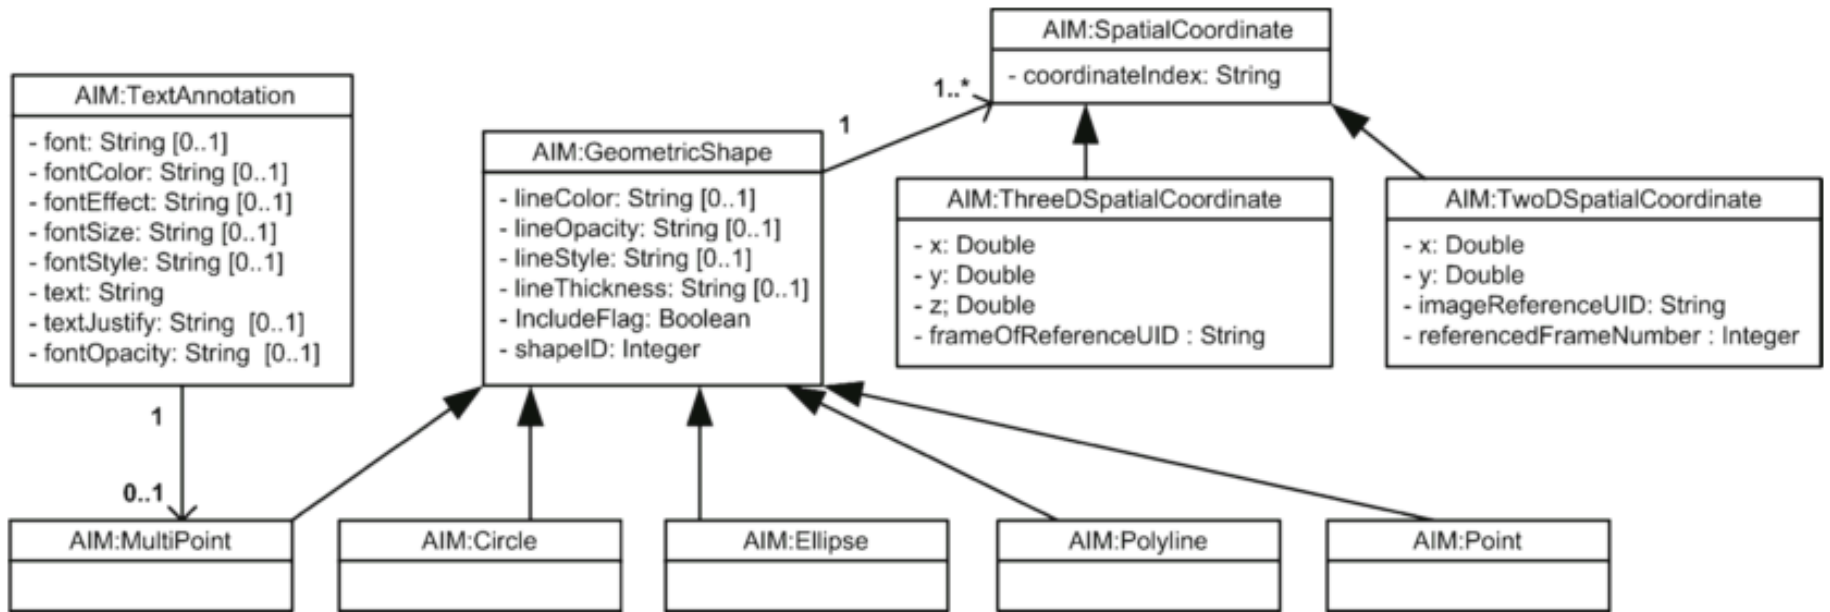


Fig 5. Markup group.

Annotation templates


- The AIM template XML schema allows to create an XML document containing controlled questions and answers based on known vocabularies such as SNOMED CT, RadLex, LOINC, etc. as well as user-defined terminologies.
- DICOM SR templates – similar purpose, vocabularies

Example

RANO Template

```
<?xml version="1.0" encoding="UTF-8"?>
<TemplateContainer authors="oslo_mgh" name="RANO NEW"
  version="1.0" description="RANO WITHOUT MEASURABLE DISEASE ASSESSMENT"
  creationDate="2011-11-18" xsi:schemaLocation="gme://caCORE.caCORE/3.2/edu.northwestern.radiology.AIMTemplate AIMTemplate_v1rv18.xsd"
  xmlns="gme://caCORE.caCORE/3.2/edu.northwestern.radiology.AIMTemplate"
  xmlns:xsi="http://www.w3.org/2001/XMLSchema-instance">
  <Template name="RANO_NEW" version="1.0" authors="oslo_mgh"
    description="Response Assessment in Neuro-Oncology" uid="123.987.32156.8454.1213156464.87987"
    codeValue="RANO" codeMeaning="Response Assessment in Neuro-Oncology" codingSchemeDesignator="RANO"
    creationDate="2011-11-18">
    <Component label="2-Non-Measurable Disease" minCardinality="1" maxCardinality="1" itemNumber="1" shouldDisplay="true"
      explanatoryText="Evaluation of Non-Measurable Disease" authors="mcpinho77">
      <Inference annotatorConfidence="false"/>
      <AllowedTerm codeMeaning="Stable Disease" codeValue="RANO1" codingSchemeDesignator="RANO">
      </AllowedTerm>
      <AllowedTerm codeMeaning="Progressive Disease" codeValue="RANO4" codingSchemeDesignator="RANO">
      </AllowedTerm>
      <AllowedTerm codeMeaning="Baseline" codeValue="RANO0" codingSchemeDesignator="RANO">
      </AllowedTerm>
      <AllowedTerm codeMeaning="Not Present" codeValue="RANO5" codingSchemeDesignator="RANO">
      </AllowedTerm>
      <AllowedTerm codeMeaning="Non-evaluable" codeValue="RANO6" codingSchemeDesignator="RANO">
      </AllowedTerm>
    </Component>
    <Component label="3-FLAIR" minCardinality="1" maxCardinality="1" itemNumber="2" shouldDisplay="true"
      explanatoryText="Tumor Evaluation on FLAIR" authors="mcpinho77">
      <Inference annotatorConfidence="false"/>
      <AllowedTerm codeMeaning="Stable Disease" codeValue="RANO1" codingSchemeDesignator="RANO">
      </AllowedTerm>
      <AllowedTerm codeMeaning="Progressive Disease" codeValue="RANO4" codingSchemeDesignator="RANO">
      </AllowedTerm>
      <AllowedTerm codeMeaning="Baseline" codeValue="RANO0" codingSchemeDesignator="RANO">
      </AllowedTerm>
      <AllowedTerm codeMeaning="Not Present" codeValue="RANO5" codingSchemeDesignator="RANO">
      </AllowedTerm>
      <AllowedTerm codeMeaning="Non-evaluable" codeValue="RANO6" codingSchemeDesignator="RANO">
      </AllowedTerm>
    </Component>
    <Component label="1-Measurable Disease" minCardinality="1" maxCardinality="1" itemNumber="0"
      shouldDisplay="true" explanatoryText="Presence or Absence of Measurable Lesions" authors="mcpinho77">
      <Inference annotatorConfidence="false"/>
      <AllowedTerm codeMeaning="Yes" codeValue="RANO7" codingSchemeDesignator="RANO">
      </AllowedTerm>
      <AllowedTerm codeMeaning="No" codeValue="RANO8" codingSchemeDesignator="RANO">
      </AllowedTerm>
      <AllowedTerm codeMeaning="Not Evaluable" codeValue="RANO6" codingSchemeDesignator="RANO">
      </AllowedTerm>
    </Component>
  </Template>
</TemplateContainer>
```

ClearCanvas TCGA WS



The image displays the ClearCanvas TCGA WS interface. On the left, an axial MRI scan of a brain is shown. A yellow dashed line indicates a measurement of 7.14 cm for a lesion. The text "BreastDx-01-0068_andrey_2012-01-09 19:09 PM" is overlaid on the scan. The scan is labeled "A" at the top and "P" at the bottom. A scale bar is visible at the bottom of the scan area.

On the right, the "AIM Annotation" panel is open. It features a dropdown menu for "AIM Template" set to "Response Assessment in Neuro-Oncology(RANO)". The "Annotation Name" field contains "BreastDx-01-0068_andrey_2012-01-09 23:59 PM". The panel includes three sections for disease assessment:

- 1-Measurable Disease:** Set to "Yes".
- 2-Non-Measurable Disease:** Set to "Progressive Disease".
- 3-FLAIR:** Set to "Stable Disease".

AIM Annotation

```
<?xml version="1.0" encoding="UTF-8" standalone="no" ?>  
<ImageAnnotation xmlns="gme://caCORE.caCORE/3.2/  
edu.northwestern.radiology.AIM" aimVersion="3.0"  
cagridId="0" codeMeaning="Response Assessment in Neuro-  
Oncology" codeValue="RANO"  
codingSchemeDesignator="RANO"  
dateTime="2012-01-09T19:09:58"  
name="BreastDx-01-0068_andrey_2012-01-09 19:09 PM"  
uniqueIdentifier="1.3.6.1.4.1.25403.8796750565674.2788.20  
120109070958.2" xmlns:xsi="http://www.w3.org/2001/  
XMLSchema-instance" xsi:schemaLocation="gme://  
caCORE.caCORE/3.2/edu.northwestern.radiology.AIM  
AIM_v3_rv11_XML.xsd">
```


AIM Annotation cont.

```
<calculationCollection>
  <Calculation cagridId="0" codeMeaning="Length" codeValue="G-A22A" codingSchemeDesignator="SRT" description="Length"
uid="1.3.6.1.4.1.25403.8796750565674.2788.20120109070958.1">
  <referencedCalculationCollection/>
  <calculationResultCollection>
    <CalculationResult cagridId="0" numberOfDimensions="1" type="Scalar" unitOfMeasure="mm">
      <calculationDataCollection>
        <CalculationData cagridId="0" value="71.3865693161104">
          <coordinateCollection>
            <Coordinate cagridId="0" dimensionIndex="0" position="0"/>
          </coordinateCollection>
        </CalculationData>
      </calculationDataCollection>
      <dimensionCollection>
        <Dimension cagridId="0" index="0" label="Value" size="1"/>
      </dimensionCollection>
    </CalculationResult>
  </calculationResultCollection>
  <referencedGeometricShapeCollection>
    <ReferencedGeometricShape cagridId="0" referencedShapeIdentifier="0"/>
  </referencedGeometricShapeCollection>
</Calculation>
</calculationCollection>
```

AIM Annotation cont.

```
<inferenceCollection>
  <Inference cagridId="0" codeMeaning="Yes" codeValue="RANO7" codingSchemeDesignator="RANO" codingSchemeVersion="" imageEvidence="true"/>
  <Inference cagridId="0" codeMeaning="Progressive Disease" codeValue="RANO4" codingSchemeDesignator="RANO" codingSchemeVersion="" imageEvidence="true"/>
  <Inference cagridId="0" codeMeaning="Stable Disease" codeValue="RANO1" codingSchemeDesignator="RANO" codingSchemeVersion="" imageEvidence="true"/>
</inferenceCollection>

<user>
  <User cagridId="0" loginName="andrey" name="andrey" numberWithinRoleOfClinicalTrial="1" roleInTrial="Performing"/>
</user>

<equipment>
  <Equipment cagridId="0" manufacturerModelName="AIM_TCGA_v3" manufacturerName="Northwestern University" softwareVersion="3.0.0.3"/>
</equipment>

<imageReferenceCollection>
  <ImageReference cagridId="0" xsi:type="DICOMImageReference">
    <imageStudy>
      <ImageStudy cagridId="0" instanceUID="1.3.6.1.4.1.14519.5.2.1.4792.2001.200235584781096359647374535914" startDate="2008-06-27T00:00:00"
startTime="000000">
        <imageSeries>
          <ImageSeries cagridId="0" instanceUID="1.3.6.1.4.1.14519.5.2.1.4792.2001.170977198031148408225883336860">
            <imageCollection>
              <Image cagridId="0" sopClassUID="1.2.840.10008.5.1.4.1.1.4" sopInstanceUID="1.3.6.1.4.1.14519.5.2.1.4792.2001.149982482708499901857882575988"/>
            </imageCollection>
          </ImageSeries>
        </imageSeries>
      </ImageStudy>
    </imageStudy>
  </ImageReference>
</imageReferenceCollection>
```

AIM Annotation cont.

```
<geometricShapeCollection>
  <GeometricShape cagridId="0" includeFlag="true" shapeIdentifier="0" xsi:type="MultiPoint">
    <spatialCoordinateCollection>
      <SpatialCoordinate cagridId="0" coordinateIndex="0"
imageReferenceUID="1.3.6.1.4.1.14519.5.2.1.4792.2001.149982482708499901857882575988"
referencedFrameNumber="1" x="170.666656494141" xsi:type="TwoDimensionSpatialCoordinate"
y="359.489318847656"/>
      <SpatialCoordinate cagridId="0" coordinateIndex="1"
imageReferenceUID="1.3.6.1.4.1.14519.5.2.1.4792.2001.149982482708499901857882575988"
referencedFrameNumber="1" x="274.156005859375" xsi:type="TwoDimensionSpatialCoordinate"
y="337.702087402344"/>
    </spatialCoordinateCollection>
  </GeometricShape>
</geometricShapeCollection>

<person>
  <Person cagridId="0" id="BreastDx-01-0068" name="" sex="F"/>
</person>

</ImageAnnotation>
```

Corresponding DICOM SR

Dicom-File-Format

Dicom-Meta-Information-Header

Used TransferSyntax: Little Endian Explicit

(0002,0000) UL 200 # 4, 1 FileMetaInformationGroupLength
(0002,0001) OB 00\01 # 2, 1 FileMetaInformationVersion
(0002,0002) UI =ComprehensiveSRStorage # 30, 1 MediaStorageSOPClassUID
(0002,0003) UI [1.2.276.0.7230010.3.1.4.768493426.2904.1326154540.4] # 52, 1 MediaStorageSOPInstanceUID
(0002,0010) UI =LittleEndianExplicit # 20, 1 TransferSyntaxUID
(0002,0012) UI [1.2.276.0.7230010.3.0.3.5.4] # 28, 1 ImplementationClassUID
(0002,0013) SH [OFFIS_DCMTK_354] # 16, 1 ImplementationVersionName

Dicom-Data-Set

Used TransferSyntax: Little Endian Explicit

(0008,0005) CS [ISO_IR 100] # 10, 1 SpecificCharacterSet
(0008,0012) DA [20120109] # 8, 1 InstanceCreationDate
(0008,0013) TM [191540] # 6, 1 InstanceCreationTime
(0008,0014) UI [1.2.276.0.7230010.3.0.3.5.4] # 28, 1 InstanceCreatorUID
(0008,0016) UI =ComprehensiveSRStorage # 30, 1 SOPClassUID
(0008,0018) UI [1.2.276.0.7230010.3.1.4.768493426.2904.1326154540.4] # 52, 1 SOPInstanceUID
(0008,0020) DA (no value available) # 0, 0 StudyDate
(0008,0023) DA [20120109] # 8, 1 ContentDate
(0008,0030) TM (no value available) # 0, 0 StudyTime
(0008,0033) TM [191540] # 6, 1 ContentTime
(0008,0050) SH (no value available) # 0, 0 AccessionNumber
(0008,0060) CS [SR] # 2, 1 Modality
(0008,0070) LO [Northwestern University] # 24, 1 Manufacturer
(0008,0090) PN (no value available) # 0, 0 ReferringPhysicianName
(0008,103e) LO [AIM DICOM SR] # 12, 1 SeriesDescription
(0008,1090) LO [AIM_TCGA_v3] # 12, 1 ManufacturerModelName
(0008,1111) SQ (Sequence with explicit length #=0) # 0, 1 ReferencedPerformedProcedureStepSequence
(ffff,e0dd) na (SequenceDelimitationItem for re-encod.) # 0, 0 SequenceDelimitationItem
(0010,0010) PN (no value available) # 0, 0 PatientName
(0010,0020) LO [BreastDx-01-0068] # 16, 1 PatientID
(0010,0030) DA (no value available) # 0, 0 PatientBirthDate
(0010,0040) CS [F] # 2, 1 PatientSex
(0010,2160) SH (no value available) # 0, 0 EthnicGroup
(0018,1020) LO [3.0.0.3] # 8, 1 SoftwareVersions
(0020,000d) UI [1.3.6.1.4.1.14519.5.2.1.4792.2001.200235584781096359647374535914] # 64, 1 StudyInstanceUID
(0020,000e) UI [1.2.276.0.7230010.3.1.3.768493426.2904.1326154540.5] # 52, 1 SeriesInstanceUID
(0020,0010) SH (no value available) # 0, 0 StudyID
(0020,0011) IS [1] # 2, 1 SeriesNumber
(0020,0013) IS [1] # 2, 1 InstanceNumber
(0040,a040) CS [CONTAINER] # 10, 1 ValueType
(0040,a043) SQ (Sequence with explicit length #=1) # 70, 1 ConceptNameCodeSequence

Common needs ?

- Direct IO or DICOM module?
- Connection of DICOM image UIDs with Slicer volumes ?